


AD630351

RECIPROCITY CALIBRATION IN A TUBE
WITH ACTIVE-IMPEDANCE TERMINATION

Louis G. Beatty

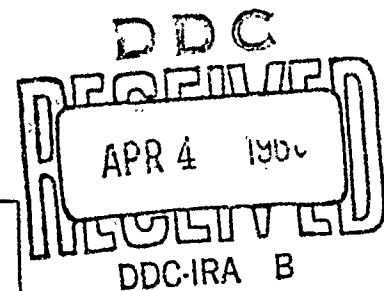

CLEARINGHOUSE
FOR FEDERAL SCIENTIFIC AND
TECHNICAL INFORMATION

Hardcopy	Microfiche	
\$ —	\$ —	11 pp as

ARCHIVE COPY

Department of the Navy *code 1, 20* Office of Naval Research

UNDERWATER SOUND REFERENCE LABORATORY

P. O. Box 8337

Orlando, Florida

Distribution of this document is unlimited



Reciprocity Calibration in a Tube with Active-Impedance Termination

LOUIS G. BEATTY

U. S. Navy Underwater Sound Reference Laboratory, Orlando, Florida 32806

A new application of the reciprocity principle has been developed for calibrating electroacoustic transducers in a closed vessel at static pressures to 8500 psi and frequencies from 100 to 1500 Hz. The necessary plane progressive wavefield is provided by sound propagation in the longitudinal mode within a sound channel terminated at both ends with active impedances. The technique is particularly well suited to the calibration of underwater-sound transducers because the high static pressure under which many of them must operate, as well as their size, mechanical construction, and operating frequency, often prevents the use of more conventional methods. The case of a rigid-walled, water-filled tube is analyzed theoretically. Results of measurements made by this method in a practical high-pressure calibration chamber are shown.

INTRODUCTION

RECIPROCITY methods, because of their basic simplicity and inherent accuracy, offer a highly attractive technique for obtaining absolute calibrations of electroacoustic devices. On the other hand, calculating the appropriate reciprocity parameter usually requires the assumption that the acoustic field satisfy rather idealized boundary conditions that often cannot be approximated closely enough in practice. This situation exists in the calibration of underwater-sound transducers at the lower end of the audio-frequency range where it is often necessary to control the ambient temperature and static pressure and where the dimensions of the measurement chamber cannot be made small in comparison with the wavelength in the water, nor can reflections from the walls be eliminated with pulsing techniques or passive absorbers.

The coupler-reciprocity technique can be used at low audio frequencies, but it is applicable only to specially constructed probe hydrophones of high mechanical impedance. It cannot be used to calibrate other transducers of different size, shape, and type of construction.

The reciprocity procedure described here was developed to provide some relief from these problems. It is well-suited for use in a cylindrical vessel of high wall stiffness and moderate internal diameter. These characteristics are compatible with the requirement that the chamber accommodate a wide variety of transducer types and configurations and withstand high static pressure. Such a tube and its use for calibration

purposes are described in a companion paper.¹ It is the purpose of this paper to present theoretical justification for the procedures.

The basic condition for valid calibration measurements in the tube is the existence of plane progressive waves in certain regions along the length of the tube. This condition is achieved by application of the principle of active impedance termination,² wherein the phase and amplitude of the electrical signal driving a transducer are varied relative to the phase and amplitude of the acoustic signal that it receives from a source transducer. The first transducer can be made to act as a controllable acoustic impedance with respect to the received signal. The reciprocity parameter applicable to the procedure is the plane-wave parameter first derived by Simmons and Urick,³ where the area of the plane wave is the cross-sectional area of the channel.


In the analysis that follows, it is assumed that the walls of the calibration chamber are rigid and that the chamber is filled with airfree water and is excited by a sinusoidal signal in the frequency range for which only the longitudinal mode of sound propagation occurs in

¹ L. G. Beatty, R. J. Bobber, and David L. Phillips, "Sonar Transducer Calibration in a High-Pressure Tube," *J. Acoust. Soc. Am.* 39, 48-54 (1966).

² L. G. Beatty, "Acoustic Impedance in a Rigid-Walled Cylindrical Sound Channel Terminated at Both Ends with Active Transducers," *J. Acoust. Soc. Am.* 36, 1081-1089 (1964).

³ B. D. Simmons and R. J. Urick, "The Plane Wave Reciprocity Parameter and Its Application to the Calibration of Electroacoustic Transducers at Close Distances," *J. Acoust. Soc. Am.* 21, 633-635 (1949).

FIG. 1. Experimental arrangement.

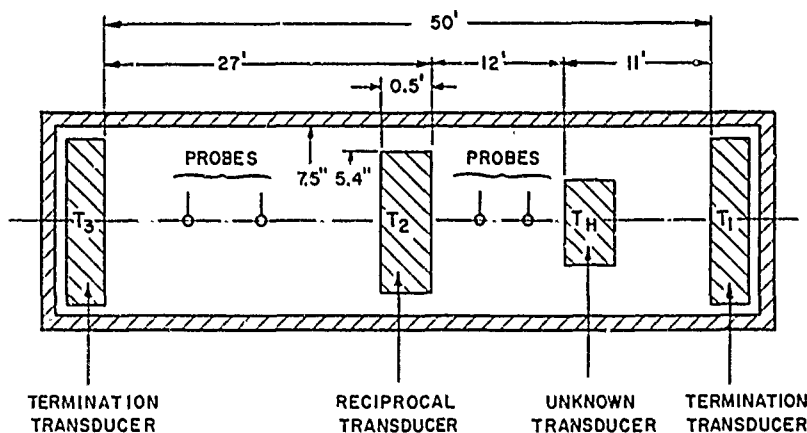

the water without attenuation. These conditions can be approximated satisfactorily in a thick-walled steel tube of internal radius b that satisfies the requirement

$$b \leq c/5f, \quad (1)$$

where f is the highest operating frequency desired and c is the longitudinal speed of sound in the water. The length of the chamber must be sufficient at all operating frequencies to ensure that there are two regions within the medium where only plane-wave components of the field exist. Further, each of the regions should extend at least the distance $\lambda/4$ at the frequency of measurement to ensure sufficient sensitivity in the detection of the plane progressive wave. This requirement is somewhat analogous to the criterion for spherical-wave reciprocity—that measurements are to be made at a sufficiently large distance from the reciprocal transducer to ensure that spherical-wave propagation exist there.

I. MEASUREMENT PROCEDURE

Three transducers and four or more probe hydrophones are used in the measurement process. One of the transducers must be reciprocal and must satisfy certain impedance requirements, which are discussed later. The probe hydrophones serve to monitor the wave-propagation conditions in the tube. Preferably, the number and spacing of these probes should be such as to allow a good sampling of the conditions at all frequencies of interest. In measurements at the U. S. Navy Underwater Sound Reference Laboratory (USRL), nine probe hydrophones are spaced at various multiples of 1 ft along the axis of the chamber in the regions of interest.

The procedure follows that of the conventional reciprocity calibration, with the exception that conditions in the tube must be adjusted during each set of measurements to obtain plane progressive waves throughout certain regions of the chamber. Consider the physical arrangement depicted in Fig. 1, where T_2 is the reciprocal transducer and T_H is the transducer that is used strictly as a receiver. First, transducer T_1 is driven while T_2 receives; next, T_1 serves as the termi-

nation transducer while T_2 is driven. Transducer T_3 serves solely as a termination device in both cases. The "double termination" procedure, so called because the terminal impedances at both ends of the tube are controlled when the reciprocal transducer is driving the tube, consists of the following steps.

1. Drive T_1 and T_3 at the same frequency, leaving T_2 open-circuited. Adjust the magnitude and phase relationships of the currents driving T_1 and T_3 so that plane progressive waves traveling toward T_2 are obtained in the region between T_H and T_2 , this condition being detected by probe hydrophones removed far enough from T_H and T_2 to be out of the regions of field divergence associated with these transducers. Under these conditions, measure the open-circuit output voltages E_{2r} of T_2 and E_{Hr} of T_H . The method by which the required progressive-wave condition is detected with the probe hydrophones is discussed in detail in the companion paper¹; in general, however, it involves the establishment of a particular phase-and-amplitude relationship between the outputs of a suitably chosen pair of probes.

2. Drive T_2 , T_1 , and T_3 , adjusting the phase and amplitude relationships of the currents into T_1 and T_3 relative to the current into T_2 so that plane progressive waves again are obtained simultaneously in the regions between T_2 and T_H traveling toward T_H and between T_2 and T_3 traveling toward T_3 . Thus, the reciprocal source transducer is radiating into a doubly terminated channel. Measure the current I_{2s} driving T_2 and the open-circuit voltage E_{Hs} of T_H .

The values obtained for these parameters can be used now in the normal reciprocity equation to calculate the tube transmitting current response or voltage sensitivity of T_2 , or the voltage sensitivity of T_H , which, within prescribed limitations, will be equivalent to the free-field values. The voltage sensitivity M_H of T_H is

$$M_H = \left[\frac{E_{Hr} E_{Hs}}{E_{2r} I_{2s}} J_t \right]^{1/2}, \quad (2)$$

where J_t is the reciprocity parameter in the tube. It is

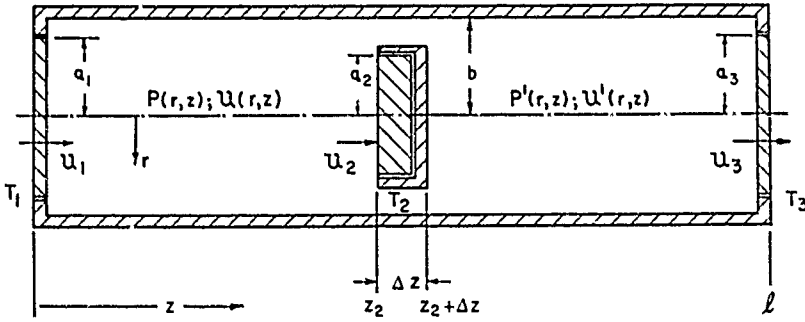


FIG. 2. Mathematical model.

shown in Sec. II-C1 that, for the prescribed measurement conditions and for certain limitations on the impedance of the reciprocal transducer,

$$|J_t| = 2A_t/\rho c, \quad (3)$$

where A_t is the cross-sectional area of the tube and ρ is the density of the water in the tube.

Another, less-useful, arrangement is called "single termination." When this arrangement is used, Step 2 is changed to allow T_3 to be passive and open-circuited. Plane progressive waves are then present only in the region between T_H and T_2 , traveling toward T_H .

The magnitude of the reciprocity parameter for this case is

$$|J_t'| = A_t/\rho c |\cos \theta|, \quad (4)$$

where θ is an angle determined by the frequency and the distance between T_2 and T_3 . This form of the reciprocity parameter, derived in Sec. II-C2, also imposes restrictions on the impedance of the reciprocal transducer and further imposes certain conditions on the effective acoustic impedance of T_3 , open-circuited, to the plane-wave mode in the water in the tube.

II. THEORY

A. Solution of the Wave Equation

The derivations that follow are based on rather simple boundary conditions. In general, these simplifications do not restrict the practical application of the technique, provided that the basic assumptions of reciprocity are satisfied in practice and plane progressive waves are obtained.

Consider the mathematical model of Fig. 2 and assume the following conditions. The system consists of a rigid-walled, water-filled tube, of radius b and length l , that is driven by coaxial transducers T_1 , T_2 , and T_3 , whose diaphragms are pistons of radii a_1 , a_2 , and a_3 , respectively. The face of transducer T_1 is at $z=0$; T_2 , at $z=z_2$, facing T_1 ; T_3 , at $z=l$, faces the back of T_2 , which is considered rigid. Denote the piston velocities of the transducers by U_1 , U_2 , and U_3 . The over-all thickness Δz of T_2 in the z direction is assumed to be small enough that its effect on the solution can be neglected.

The general solution of the wave equation for the

system is considered to consist of the following parts:

$$\phi(r,z) = \sum_{n=0}^{\infty} [\alpha_n \exp(-\sigma_n z) + \beta_n \exp(\sigma_n z)] J_0(\kappa_n r) \quad (5)$$

for $0 \leq z \leq z_2$, and

$$\phi'(r,z) = \sum_{n=0}^{\infty} [\alpha'_n \exp(-\sigma_n z) + \beta'_n \exp(\sigma_n z)] J_0(\kappa_n r) \quad (6)$$

for $(z_2 + \Delta z) \leq z \leq l$. In these expressions, $\phi(r,z)$ and $\phi'(r,z)$ represent the usual velocity potential functions having the common phase propagation constant $\sigma_n = (\kappa_n^2 + k^2)^{1/2}$, where κ_n and k are the radial and longitudinal components, respectively, of σ_n . The longitudinal component is related to the excitation frequency by $k = \omega/c$, where $\omega = 2\pi f$, f being the excitation frequency. The constants α_n , α'_n , β_n , and β'_n are amplitude coefficients of ϕ and ϕ' . The radial dependency is determined by $J_0(\kappa_n r)$, the zero-order Bessel function of argument $(\kappa_n r)$, symmetry with respect to the z axis having been assumed.

The constant κ_n relates to the radial mode of wave propagation within the water. Its value is determined by the requirement that the radial velocity be zero at the walls of the tube; that is, the boundary condition

$$-\partial\phi/\partial r = -\partial\phi'/\partial r = 0 \quad \text{for } r=b, \quad (7)$$

which is satisfied in both solutions by the same value of κ_n : namely,

$$\kappa_n = j_n/b; \quad n=0, 1, 2, 3, \dots, \quad (8)$$

where j_n is the n th zero of the first-order Bessel equation.

The remaining boundary conditions to be satisfied are

$$-\frac{\partial\phi}{\partial z} = \begin{cases} U_1 & \text{for } 0 \leq r \leq a_1, \\ 0 & \text{for } a_1 < r \leq b, \end{cases} \quad z=0; \quad (9)$$

$$-\frac{\partial\phi}{\partial z} = \begin{cases} U_2 & \text{for } 0 \leq r \leq a_2, \\ U(r, z_2) & \text{for } a_2 < r \leq b, \end{cases} \quad z=z_2; \quad (10)$$

$$-\frac{\partial\phi'}{\partial z} = \begin{cases} 0 & \text{for } 0 \leq r \leq a_2, \\ U(r, z_2 + \Delta z) & \text{for } a_2 < r \leq b, \end{cases} \quad z=z_2 + \Delta z; \quad (11)$$

$$-\frac{\partial\phi'}{\partial z} = \begin{cases} U_3 & \text{for } 0 \leq r \leq a_3, \\ 0 & \text{for } a_3 < r \leq b, \end{cases} \quad z=l; \quad (12)$$

where $U(r, z)$ is the longitudinal particle velocity at point (r, z) .

Because the conditions expressed by Eqs. 10 and 11 are not independent, an additional set of relationships is required. This set is obtained from the force equations over the regions $a_2 < r \leq b$ at $z = z_2$ and $z_2 + \Delta z$:

$$F(z_2) = i2\pi\omega\rho \int_{a_2}^b \phi(r, z_2) r dr, \quad (13)$$

$$F(z_2 + \Delta z) = i2\pi\omega\rho \int_{a_2}^b \phi'(r, z_2 + \Delta z) r dr, \quad (14)$$

where, as usual, $i = \sqrt{-1}$.

From these boundary relationships and the assumption that $z_2 \approx z_2 + \Delta z$, the following expressions are obtained for the constants α_n , α'_n , β_n , and β'_n :

$$\alpha_n = (S_n j_n / i4\pi\rho\omega b) [U_3 a_3 J_3 + U_2 a_2 J_2 \cosh \sigma_n(l - z_2) - U_1 a_1 J_1 \exp(\sigma_n l)], \quad (15)$$

$$\alpha'_n = (S_n j_n / i4\pi\rho\omega b) [U_3 a_3 J_3 + (U_2 a_2 J_2 \cosh \sigma_n z_2 - U_1 a_1 J_1) \exp(\sigma_n l)], \quad (16)$$

$$\beta_n = (S_n j_n / i4\pi\rho\omega b) [U_3 a_3 J_3 + U_2 a_2 J_2 \cosh \sigma_n(l - z_2) - U_1 a_1 J_1 \exp(-\sigma_n l)], \quad (17)$$

$$\beta'_n = (S_n j_n / i4\pi\rho\omega b) [U_3 a_3 J_3 + (U_2 a_2 J_2 \cosh \sigma_n z_2 - U_1 a_1 J_1) \exp(-\sigma_n l)], \quad (18)$$

where

$$S_n \equiv -i4\pi\rho\omega / \sigma_n j_n^2 J_0^2(j_n) \sinh \sigma_n l, \quad (19)$$

$$J_1 \equiv J_1(a_1 j_n / b), \quad J_2 \equiv J_1(a_2 j_n / b), \quad J_3 \equiv J_1(a_3 j_n / b),$$

and J_1 on the right-hand side of these expressions for J_1 , J_2 , and J_3 indicates the Bessel function of order one and argument indicated in the parentheses.

B. Related Force Equations

The relation of the field equations to the driving forces F_1 , F_2 , and F_3 , applied to transducers T_1 , T_2 , and T_3 by their electrical currents is obtained by considering the transducers to be driven by Thévenin generators of internal mechanical impedances Z_{1m} , Z_{2m} , and Z_{3m} . The following equations can be written for this condition:

$$F_1 = U_1 [K_{10} + (U_2/U_1)K_{12} + (U_3/U_1)K_{13}], \quad (20)$$

$$F_2 = U_2 [K_{20} + (U_1/U_2)K_{21} - (U_2/U_2)K_{23}], \quad (21)$$

$$F_3 = U_3 [K_{30} + (U_1/U_3)K_{31} - (U_2/U_3)K_{32}], \quad (22)$$

where $K_{10} \equiv Z_{1m} - K_{11}$, $K_{20} \equiv Z_{2m} - K_{22}$, $K_{30} \equiv Z_{3m} - K_{33}$, and the terms K_{pq} ($p, q = 1, 2, 3$) represent the interaction impedance functions (in mechanical units) of the acoustical system associated with transducers T_1 ,

T_2 , and T_3 , as follows:

$$\begin{aligned} K_{11} &\equiv a_1^2 \sum_{n=0}^{\infty} S_n J_1^2 \cosh \sigma_n l, \\ K_{22} &\equiv a_2^2 \sum_{n=0}^{\infty} S_n J_2^2 \cosh \sigma_n(l - z_2) \cosh \sigma_n z_2, \\ K_{33} &\equiv a_3^2 \sum_{n=0}^{\infty} S_n J_3^2 \cosh \sigma_n l, \end{aligned} \quad (23)$$

$$K_{12} = K_{21} \equiv a_1 a_2 \sum_{n=0}^{\infty} S_n J_1 J_2 \cosh \sigma_n(l - z_2),$$

$$K_{13} = K_{31} \equiv a_1 a_3 \sum_{n=0}^{\infty} S_n J_1 J_3,$$

$$K_{23} = K_{32} \equiv a_2 a_3 \sum_{n=0}^{\infty} S_n J_2 J_3 \cosh \sigma_n z_2.$$

C. Derivation of the Reciprocity Parameter

The preceding equations, in association with the measurement conditions previously outlined, now can be used to derive the reciprocity parameter for the tube. In the derivations that follow, for convenience, we use the superscript notation 0 to indicate that the series terms involved in the expressions contain only the terms for which $n=0$, and the superscript $n+1$ to indicate that the series terms are formed from $n+1$ to ∞ . Also, we use the symbols A_1 , A_2 , A_3 , and A_t to indicate the areas of the diaphragms of the projectors and the cross-sectional area of the tube bore.

1. Double Termination

For Step 1 of the double-termination measurement procedure, the reciprocal transducer T_2 acts as an open-circuited receiver so that $F_2 = 0$; hence, from Eq. 21,

$$U_{2r} = [-U_{1r}K_{21} + U_{3r}K_{23}] / K_{20}, \quad (24)$$

where the subscript r indicates the receiving condition. Also, for this condition, the β_0 term, Eq. 17, equals zero, which requires that

$$A_3 U_{3r} / A_2 U_{2r} - (A_1 U_{1r} / A_2 U_{2r}) e^{-ikl} = -\cosh k(l - z_2). \quad (25)$$

The force equation in the region $0 \leq z \leq z_2$ over the area A_2 can be expressed as the sum


$$F_r(z, A_2) = F_r^0(z, A_2) + F_r^{n+1}(z, A_2). \quad (26)$$

In terms of the plane progressive-wave pressure $P_r^0(z)$, it can be shown that

$$P_r^0(z) = (1/A_2) F_r^0(z, A_2) = A_1 Z_0 U_{1r} e^{ikz}, \quad (27)$$

where $Z_0 = \rho c / A_t$.

Finally, for the imposed conditions, the effect of mutual interaction of the higher-order modes among the transducers can be neglected in the interaction

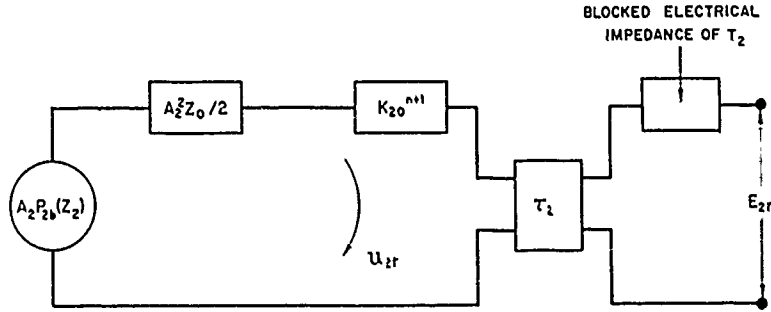FIG. 3. Electrical analog circuit of transducer T_2 as receiver.

impedance functions; that is, we can use the approximations

$$K_{pq}^{n+1} (p \neq q) \approx 0. \quad (28)$$

These results can be used to put Eq. 24 in the form

$$U_{2r} = A_2 P_r^0(z_2) / K_{20}^{n+1}. \quad (29)$$

Now, T_2 can be represented as a receiver by the electrical analog circuit shown in Fig. 3, where the Thévenin generator pressure or blocked pressure over the area A_2 has been labeled $P_{2b}(z_2)$. This blocked pressure is proportional to the plane progressive-wave pressure $P_r^0(z_2)$; that is,

$$P_{2b}(z_2) = D_{2t} P_r^0(z_2), \quad (30)$$

where D_{2t} is a constant. In a free field, this constant is called the diffraction constant of the transducer and normally is considered to be a function of the shape, dimensions relative to the wavelength of sound in the acoustic medium, and the orientation of the transducer in the sound field. In the tube, the constant D_{2t} , which will be called the tube diffraction constant of transducer T_2 , not only is a function of these parameters, but it depends upon the mechanical impedance of the transducer as well.

To obtain the expression for D_{2t} , we note from Fig. 3 and Eq. 30 that

$$U_{2r} = A_2 D_{2t} P_r^0(z_2) / (\frac{1}{2} A_2^2 Z_0 + K_{20}^{n+1}). \quad (31)$$

Equating the right-hand members of Eqs. 29 and 31 and solving for D_{2t} gives

$$D_{2t} = 1 + \frac{1}{2} A_2^2 Z_0 / K_{20}^{n+1}. \quad (32)$$

By definition, the receiving sensitivity M_2 of T_2 is

$$M_2 = E_{2r} / P_r^0(z_2) = U_{2r} \tau_2 / P_r^0(z_2), \quad (33)$$

where τ_2 is the electromechanical transfer constant of transducer T_2 .

Thus, through the use of Eq. 31,

$$M_2 = A_2 D_{2t} \tau_2 / (\frac{1}{2} A_2^2 Z_0 + K_{20}^{n+1}). \quad (34)$$

For the transmission conditions of Step 2, it is required that $\alpha_0 = \beta_0 = 0$. For this condition to be satisfied, it is necessary that

$$U_{1s} / U_{2s} = \frac{1}{2} (A_2 / A_1) \exp(-ikz_2), \quad (35)$$

and

$$U_{3s} / U_{2s} = -\frac{1}{2} (A_2 / A_3) \exp[-ik(l-z_2)], \quad (36)$$

so that

$$U_{1s} / U_{3s} = - (A_3 / A_1) \exp[ik(l-2z_2)], \quad (37)$$

where the subscript S denotes the transmitting condition.

It should be noted here that solutions of the form $\alpha_0 = \alpha_0' = 0$ or $\beta_0 = \beta_0' = 0$ give rise to mathematically indeterminate forms, implying that they are physically unattainable. This, of course, merely confirms that plane progressive waves proceeding in identical directions in both sections of the tube cannot be achieved unless the physical effect of transducer T_2 can be neglected—that is, unless T_2 appears essentially as the characteristic impedance Z_0 without being driven.

For the imposed conditions, Eq. 21 can be written in the form

$$U_{2s} = F_2 / (\frac{1}{2} A_2^2 Z_0 + K_{20}^{n+1}). \quad (38)$$

The pressure in the plane progressive wave can be expressed as

$$P_s^0(z) = \frac{1}{2} Z_0 A_2 U_{2s} \exp[i\pi - k(z_2 - z)]. \quad (39)$$

By using Eqs. 38 and 39, the transmitting response of T_2 in the tube for the case of double termination can be expressed as

$$S_2 = \tau_2 (\frac{1}{2} Z_0) A_2 \exp[i\pi - k(z_2 - z)] / (\frac{1}{2} A_2^2 Z_0 + K_{20}^{n+1}) = P_s^0(z) / I_{2s}. \quad (40)$$

Now, we define the reciprocity parameter for the case of double termination as the ratio of Eq. 34 to Eq. 40:

$$J_t = M_2 / S_2 = (2D_{2t} / Z_0) \exp\{-i[\pi - k(z_2 - z)]\}. \quad (41)$$

For the imposed frequency limitations, the term $-K_{22}^{n+1}$ in the expression for D_{2t} has the form of a mass reactance iX_{22} . Hence, Eq. 32 can be written in the form

$$D_{2t} = 1 + \frac{1}{2} A_2^2 Z_0 / (Z_{2m} + iX_{22}). \quad (42)$$

The sum $\frac{1}{2} A_2^2 Z_0 + iX_{22}$ is the mechanical equivalent of the radiation load on transducer T_2 in the tube for the case of double termination, the reactive portion or the $n+1$ terms of K_{22} being attributed to the effects of divergence in the vicinity of the transducer.

Now, if we assume that the reciprocal transducer is so constructed that its mechanical impedance satisfies the condition

$$(A_2^2 \rho c / A_1) (1 / |Z_{2m} + iX_{22}|) \ll 2, \quad (43)$$

then $|D_{2t}| \approx 1$ for the tube, and the magnitude of the reciprocity parameter becomes

$$|J_t| = 2A_1 / \rho c. \quad (44)$$

This restriction, Eq. 43, implies, in practice, that the reciprocal transducer appear as a stiffness-controlled device over the frequency range of interest.

2. Single Termination

For the case of single termination, Step 2 of the measurement procedure is modified. Transducer T_3 is open-circuited instead of being driven. This condition gives rise to standing waves in the region between T_2 and T_3 , and both the reciprocity parameter and the diffraction constant are affected thereby.

The tube diffraction constant in this case takes the form

$$D_{2t}' = 1 + A_2^2 Z_0 |\cos k(l - z_2)| \exp(ikz_2) / K_{20}^{n+1}. \quad (45)$$

The receiving sensitivity, Eq. 34, becomes

$$M_2 = \tau_2 A_2 D_{2t}' / [A_2^2 Z_0 |\cos k(l - z_2)| \times \exp(ikz_2) + K_{20}^{n+1}]. \quad (46)$$

For the transmitting response, we obtain

$$S_2 = \frac{Z_0 A_2 \tau_2 \exp[ik(z - \pi)] |\cos k(l - z_2)|}{A_2^2 Z_0 |\cos k(l - z_2)| \exp(ikz_2) + K_{20}^{n+1}}, \quad (47)$$

in the derivation of which we have used the relationship obtained from Eqs. 22 and 25:

$$\frac{U_{2S}}{U_{1S}} = e^{ikl} \frac{A_1}{A_2 \cos k(l - z_2) + i(Z_0 A_3^2 / K_{30}^{n+1}) \sin k(l - z_2)} \frac{1 + Z_0 A_3^2 / K_{30}^{n+1}}{A_2 \cos k(l - z_2) + i(Z_0 A_3^2 / K_{30}^{n+1}) \sin k(l - z_2)}. \quad (48)$$

When it is assumed that $|Z_0 A_3^2 / K_{30}^{n+1}| \ll 1$, we obtain as an approximation for the magnitude of Eq. 48.

$$|U_{2S} / U_{1S}| \approx (A_1 / A_2) / |\cos k(l - z_2)|. \quad (49)$$

It should be noted that, when $\cos k(l - z_2) = 0$, the expression in Eq. 48 remains finite unless $Z_0 A_3^2 / K_{30}^{n+1}$ also is zero—that is, unless the termination transducer appears as an infinite impedance. If K_{30}^{n+1} is purely reactive, then it is also possible for the denominator to become zero for nonzero values of $\cos k(l - z_2)$. In practice, the ratio U_{2S} / U_{1S} will remain finite because of the losses always present in the real system.

We now require that

$$|A_2^2 Z_0 \cos k(l - z_2) \exp - ik(l - z_2) / K_{20}^{n+1}| \quad (50)$$

be negligibly small in comparison with 1 so that the

tube diffraction constant can be taken as approximately equal to 1, $D_{2t}' \approx 1$. Then, for the single termination,

$$|J_t'| = \frac{A_1}{Z_0} \left| \frac{1}{\cos[(\omega/c)(l - z_2)]} \right| \quad (51)$$

or

$$|J_t'| = A_1 / \rho c |\cos \theta|,$$

where $\theta = (\omega/c)(l - z_2)$.

III. COMPARISON OF TUBE RECIPROCITY AND FREE-FIELD RECIPROCITY RESULTS

Let S_t and S_f be the transmitting current responses in the tube and in the free field, respectively, and note that, if the transducer is reciprocal, the ratio of these responses is

$$S_t / S_f = (J_t / J_f) (M_t / M_f), \quad (52)$$

where M_t and M_f are the receiving responses in the free field and in the tube, and J_t and J_f are the reciprocity parameters for the free field and the tube. Equation 52 can also be written in the form

$$\frac{S_t}{S_f} = \left| \frac{Z_m + Z_{rt}}{D_t} \right| \left| \frac{D_f}{Z_m + Z_{rf}} \right| \frac{A_t f}{dc}, \quad (53)$$

where Z_{rt} and Z_{rf} are, respectively, the radiation loads in mechanical units in the tube and in the free field, d is the distance to which the free-field measurements are referred, and D_t and D_f are the diffraction constants.

For the imposed restrictions on the ratio of wavelength to transducer dimensions, $D_t \approx 1$. Thus, when D_{2t} is substituted for D_t , Eq. 53 may be expressed in the form

$$\left| \frac{S_t}{S_f} \right| = \left| \frac{Z_m + iX_{rt}}{Z_m + R_{rf} + iX_{rf}} \right| \frac{A_t f}{dc}, \quad (54)$$

where, in terms of mechanical units, X_{rt} and X_{rf} are the mass reactive portions of the radiation load in the tube and in the free field, respectively, and R_{rf} is the free-field radiation resistance.

Thus, equality between the two responses depends on the magnitude of the differences that occur in the acoustic radiation loads and on the factor $A_t f / dc$. Equality between the open-circuit voltage receiving responses depends only on the former.

For transducers operating in the stiffness-controlled portion of their frequency range, the voltage sensitivities are equal. Above resonance, the mass reactive terms in the sensitivities control. Hence, if the net change in radiation mass in the tube is small in comparison with the total free-field mass, then the two sensitivities are approximately equal in this portion of the frequency range also.

For a resonant transducer, two effects are predominant: (1) a shift occurs in the frequency of resonance in the sensitivity-versus-frequency curves, reso-

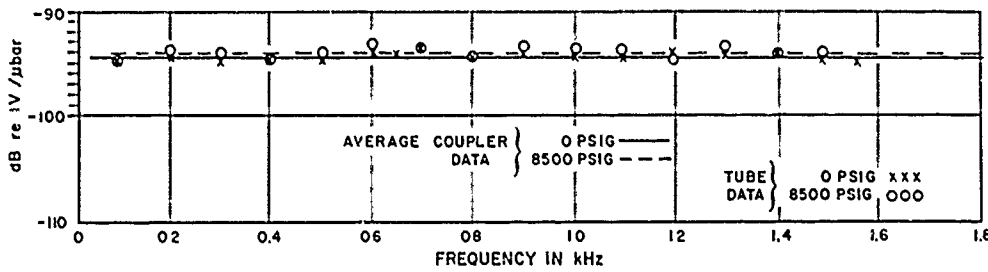


FIG. 4. Free-field voltage sensitivity, G20 hydrophone.

nance in the tube occurring at the higher frequency, and (2) a change occurs in the broadness of the peaks in the vicinity of resonance on the sensitivity curves.

Both of these changes are attributed to the differences in the radiation mass under the respective conditions. In addition, however, the change in the Q 's that is due to mass difference is opposed by the effects of R_{rt} in the free-field case.

The expressions for the Q 's are,

$$Q_t \approx f_t / (f_{2t} - f_{1t}) = 2\pi f_t (m_m + m_{rt}) / (R_m + R_{rt}), \quad (55)$$

$$Q_t \approx f_t / (f_{2t} - f_{1t}) = 2\pi f_t (m_m + m_{rt}) / R_m, \quad (56)$$

where R_m is a real portion of the mechanical impedance, m_m is the mass of the mechanical impedance, and m_{rt} and m_{rt} are the radiation mass in the tube and the free field, respectively. Also f_t , f_{1t} , f_{2t} and f_t , f_{1t} , f_{2t} are the frequencies of resonance and of the lower and upper 3-dB down points on the sensitivity curves in the free field and in the tube, respectively.

Thus, the ratio of the frequency difference between the 3-dB down points is

$$\frac{f_{2t} - f_{1t}}{f_{2t} - f_{1t}} = \left(1 + \frac{R_{rt}}{R_m}\right) \left(\frac{f_t}{f_t}\right)^2. \quad (57)$$

The factor $(1 + R_{rt}/R_m)$ represents the ratio of the tube sensitivity to the free-field sensitivity at the respective resonant frequencies. Thus, if $R_m \gg R_{rt}$, the sensitivities at these frequencies are equal.

In Eqs. 56 and 57, it has been assumed that, near resonance, the impedances involved are derivable from frequency-independent constants. For the same assumption, an approximate correlation can be obtained between the voltage sensitivities by plotting the tube results against the normalized frequency scale $f' = f(f_t/f_t)$.

On the f' scale in terms of voltage ratio in decibels, the error in the level of the tube response sensitivity will not be greater than $20 \log(f_t/f_t)$ on the slopes of the curve. At the peak, it will be $20 \log(Q_t/Q_t) + 20 \log(f_t/f_t)$.

We have discussed the case of resonant transducers without considering the fact that, to perform a reciprocity calibration, the tube diffraction constant D_{2t} must equal 1. As has been mentioned previously, this condition requires that the reciprocal transducer T_2 be nonresonant. On the other hand, this restriction does not apply to the receiving response of the unknown

transducer T_H ; hence, the fact that this transducer can be resonant is immaterial to the calibration process. The equivalence of the resonance to that in a free-field still depends, however, on the criteria previously discussed.

For the frequency limitations imposed, the magnitude of the radiation mass load of the medium on the transducer is essentially a function of the frequency, the density of the medium, and the effective piston area. The frequency is independent of variation in static pressure, and the density (when water is the medium) is virtually independent of it. Thus, differences between the voltage response measured in the tube and that measured in a free field for a particular transducer will vary little with static pressure unless the pressure affects the mechanical impedance of the transducer. It is justifiable to assume, therefore, that the changes encountered are, to a good approximation, a measure of the effect of the same pressure on the free-field response. Differences between the transmitting responses as a function of change of static pressure will likewise reflect actual effects of static pressure change on the free-field behavior of the transducer when allowance is made for the effect of pressure on sound speed in the water in the tube.

IV. EXPERIMENTAL RESULTS

The theory has been applied to practical measurements in the tube for both the single- and the double-termination conditions. The essentials of the physical arrangement are shown in Fig. 1. The termination and reciprocity transducers are oil-filled crystal units that act as stiffness-controlled piston drivers over the frequency range of interest, thus ensuring the fulfillment of the impedance requirements imposed by the theory. The value of $A_2^2 Z_0 / [A_1 |Z_{2m} + iX_{22}|]$ is estimated to be about 2×10^{-2} at 1.5 kHz.

The results of measurements made on a special hydrophone by double-termination reciprocity at 0 and 8500 psig are shown in Fig. 4. This hydrophone has been designed so that it can be calibrated also in a coupler chamber in the desired frequency range as a function of high static pressure. The results of coupler measurements as a function of frequency at static pressure also are shown in Fig. 4.

Figure 5 shows results obtained from single-termination measurements on a pressure-sensitive hydro-

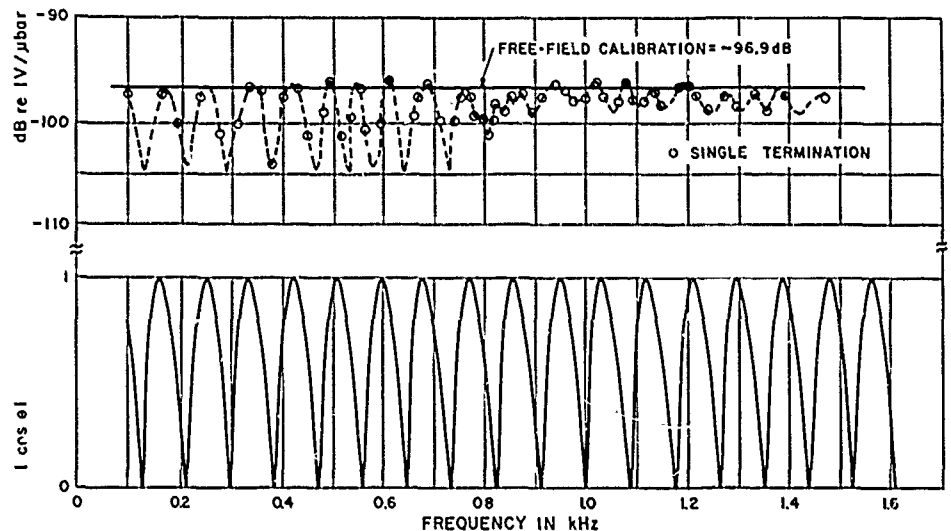


FIG. 5. Free-field voltage sensitivity by single-termination reciprocity, H35 hydrophone.

phone whose free-field response is constant within the frequency range of the measurements.

In computing the sensitivity from the single-termination measurement data, the reciprocity parameter was taken as the magnitude of the actual parameter when $\cos\theta = \pm 1$. Thus, the measured response reflects the oscillations of the reciprocity parameter.

A magnitude-versus-frequency plot of the cosine function for $(l-z_2) = 27$ ft, the distance used in the experiment, also is shown in Fig. 5. As can be seen, the period of these oscillations is in close agreement with the experimental results.

Of course, infinite terminal impedance at $z=l$ is assumed for the ideal oscillations, whereas the effective impedance of the transducer and tube closure only approximate the ideal conditions. In addition, the frequency dependence of these effective impedances results in an apparent compression and expansion of the ideal oscillation period. The cause of the rather abrupt transition in the magnitude of the oscillation starting at about 0.8 kHz has not been determined.

Additional calibration results are given in the companion paper.¹

V. CONCLUSION

A method has been described for making reciprocity calibration measurements on electroacoustic transducers under boundary conditions that, in the past, have prevented the use of the reciprocity technique. Adaptability of this technique to the case of a rigid-walled tube makes the method well suited for calibrating underwater sound transducers at various temperatures

and high static pressures and at the lower audio frequencies.

Within the imposed theoretical restrictions, the technique can be applied to resonant as well as non-resonant transducers. Theoretical justification has been given and the theory has been verified in a practical calibration facility. Results obtained are in acceptable agreement with free-field and coupler measurements.

The need for achieving plane progressive waves adds some complexity to the measurement procedure as well as to the associated electroacoustic equipment, but the measurement process is not unduly tedious. The maximum error due to failure to attain a standing-wave ratio of 1 is approximately proportional to the square root of the product of the standing-wave ratios achieved under sending and receiving conditions.

It is emphasized here that the procedures used to make absolute measurements are directly applicable to comparison calibrations also. Thus, the discussion relating measurements in the tube to those in a free field can be applied to comparison measurements as well.

ACKNOWLEDGMENTS

The author is indebted to his associates at the U. S. Navy Underwater Sound Reference Laboratory whose proficiency played a large part in the successful testing of the theories presented in this paper. Particular thanks are extended to Lynn P. Browder for the design of critical electronic circuitry, to David L. Phillips for obtaining the data, and to R. J. Bobber for his helpful review and comments.

UNCLASSIFIED

Security Classification

DOCUMENT CONTROL DATA - R&D		
(Security classification of title, body of abstract and indexing annotation must be entered when the overall report is classified)		
1. ORIGINATING ACTIVITY (Corporate author) U.S. Navy Underwater Sound Reference Laboratory P.O. Box 8337 Orlando, Florida 32806		2a. REPORT SECURITY CLASSIFICATION UNCLASSIFIED
		2b. GROUP
3. REPORT TITLE RECIPROCITY CALIBRATION IN A TUBE WITH ACTIVE-IMPEDANCE TERMINATION		
4. DESCRIPTIVE NOTES (Type of report and inclusive dates) USRL Research Report		
5. AUTHOR(S) (Last name, first name, initial) Beatty, Louis G.		
6. REPORT DATE 1 April 1966	7a. TOTAL NO. OF PAGES 8	7b. NO. OF REFS 3
8a. CONTRACT OR GRANT NO.	8a. ORIGINATOR'S REPORT NUMBER(S) USRL Research Report No. 82	
b. PROJECT NO.		
c.	8b. OTHER REPORT NO(S) (Any other numbers that may be assigned this report)	
d.		
10. AVAILABILITY/LIMITATION NOTICES Distribution of this document is unlimited		
11. SUPPLEMENTARY NOTES	12. SPONSORING MILITARY ACTIVITY	
13. ABSTRACT A new application of the reciprocity principle has been developed for calibrating electroacoustic transducers in a closed vessel at static pressures to 8500 psi and frequencies from 100 to 1500 Hz. The necessary plane progressive wavefield is provided by sound propagation in the longitudinal mode within a sound channel terminated at both ends with active impedances. The technique is particularly well suited to the calibration of underwater-sound transducers because the high static pressure under which many of them must operate, as well as their size, mechanical construction, and operating frequency, often prevents the use of more conventional methods. The case of a rigid-walled, water-filled tube is analyzed theoretically. Results of measurements made by this method in a practical high-pressure calibration chamber are shown.		

UNCLASSIFIED

Security Classification

14. KEY WORDS	LINK A		LINK B		LINK C	
	ROLE	WT	ROLE	WT	ROLE	WT
Reciprocity calibration Electroacoustic transducers Underwater sound equipment Deep-submergence transducers Measurements in a tube Measurement theory Instrumentation Active-impedance termination Acoustic waveguide						

INSTRUCTIONS

1. **ORIGINATING ACTIVITY:** Enter the name and address of the contractor, subcontractor, grantee, Department of Defense activity or other organization (*corporate author*) issuing the report.

2a. **REPORT SECURITY CLASSIFICATION:** Enter the overall security classification of the report. Indicate whether "Restricted Data" is included. Marking is to be in accordance with appropriate security regulations.

2b. **GROUP:** Automatic downgrading is specified in DoD Directive 5200.10 and Armed Forces Industrial Manual. Enter the group number. Also, when applicable, show that optional markings have been used for Group 3 and Group 4 as authorized.

3. **REPORT TITLE:** Enter the complete report title in all capital letters. Titles in all cases should be unclassified. If a meaningful title cannot be selected without classification, show title classification in all capitals in parenthesis immediately following the title.

4. **DESCRIPTIVE NOTES:** If appropriate, enter the type of report, e.g., interim, progress, summary, annual, or final. Give the inclusive dates when a specific reporting period is covered.

5. **AUTHOR(S):** Enter the name(s) of author(s) as shown on or in the report. Enter last name, first name, middle initial. If military, show rank and branch of service. The name of the principal author is an absolute minimum requirement.

6. **REPORT DATE:** Enter the date of the report as day, month, year, or month, year. If more than one date appears on the report, use date of publication.

7a. **TOTAL NUMBER OF PAGES:** The total page count should follow normal pagination procedures, i.e., enter the number of pages containing information.

7b. **NUMBER OF REFERENCES:** Enter the total number of references cited in the report.

8a. **CONTRACT OR GRANT NUMBER:** If appropriate, enter the applicable number of the contract or grant under which the report was written.

8b, 8c, & 8d. **PROJECT NUMBER:** Enter the appropriate military department identification, such as project number, subproject number, system numbers, task number, etc.

9a. **ORIGINATOR'S REPORT NUMBER(S):** Enter the official report number by which the document will be identified and controlled by the originating activity. This number must be unique to this report.

9b. **OTHER REPORT NUMBER(S):** If the report has been assigned any other report numbers (either by the originator or by the sponsor), also enter this number(s).

10. **AVAILABILITY/LIMITATION NOTICES:** Enter any limitations on further dissemination of the report, other than those

imposed by security classification, using standard statements such as:

- (1) "Qualified requesters may obtain copies of this report from DDC."
- (2) "Foreign announcement and dissemination of this report by DDC is not authorized."
- (3) "U. S. Government agencies may obtain copies of this report directly from DDC. Other qualified DDC users shall request through _____."
- (4) "U. S. military agencies may obtain copies of this report directly from DDC. Other qualified users shall request through _____."
- (5) "All distribution of this report is controlled. Qualified DDC users shall request through _____."

If the report has been furnished to the Office of Technical Services, Department of Commerce, for sale to the public, indicate this fact and enter the price, if known.

11. **SUPPLEMENTARY NOTES:** Use for additional explanatory notes.

12. **SPONSORING MILITARY ACTIVITY:** Enter the name of the departmental project office or laboratory sponsoring (paying for) the research and development. Include address.

13. **ABSTRACT:** Enter an abstract giving a brief and factual summary of the document indicative of the report, even though it may also appear elsewhere in the body of the technical report. If additional space is required, a continuation sheet shall be attached.

It is highly desirable that the abstract of classified reports be unclassified. Each paragraph of the abstract shall end with an indication of the military security classification of the information in the paragraph, represented as (TS), (S), (C), or (U).

There is no limitation on the length of the abstract. However, the suggested length is from 150 to 225 words.

14. **KEY WORDS:** Key words are technically meaningful terms or short phrases that characterize a report and may be used as index entries for cataloging the report. Key words must be selected so that no security classification is required. Identifiers, such as equipment model designation, trade name, military project code name, geographic location, may be used as key words but will be followed by an indication of technical context. The assignment of links, roles, and weights is optional.